


DIGITAL CALIPER INSTRUCTIONS

CE

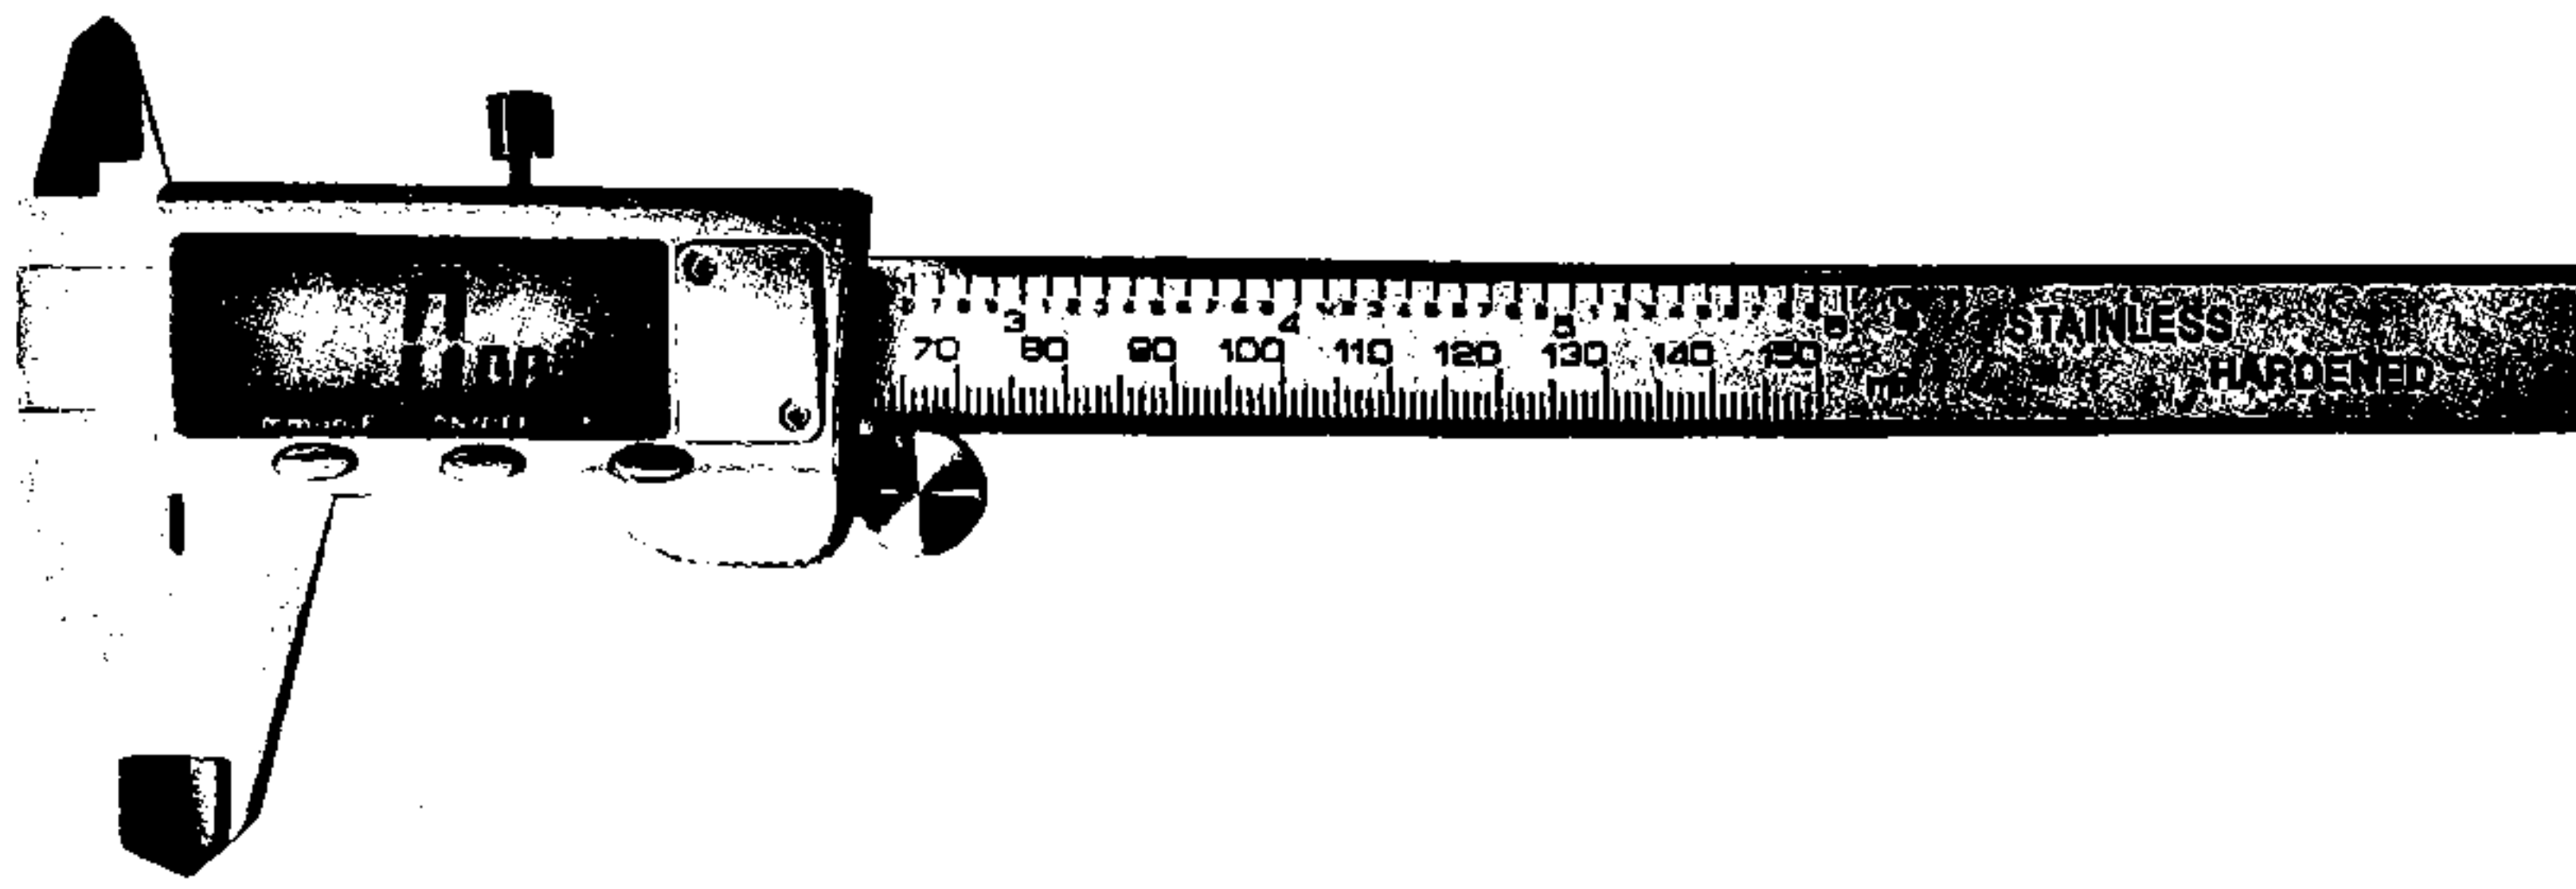

● TECHNICAL SPECIFICATIONS

Measuring range: 0-150mm/0-6", 0-200mm/0-8"
 0-300mm/1-12"
 Resolution: 0.01mm/0.0005"
 Accuracy: $\pm 0.02\text{mm}/0.001"$ ($< 100\text{mm}$)
 $\pm 0.03\text{mm}/0.001"$ ($> 100-200\text{mm}$)
 $\pm 0.04\text{mm}/0.0015"$ ($> 200-300\text{mm}$)
 Repeatability: $\pm 0.01\text{mm}/0.0005"$
 Max. measuring speed: 1.5m/sec, 60"/sec.
 Measuring system: Linear capacitive measuring system.
 Display: LCD display.
 Power: One 1.5 V button cell.
 Capacity: 165mAh
 Working temperature: 5°C-40°C/41 to 104 F.
 Influence of humidity: Not important under 80% of relative humidity.


● OPERATION

1. PREPARATIONS:


- (1) Slider can be removed only after the locking screw (No.3 item of the Nomenclature) is loosened.
- (2) Wipe clean all the measuring faces and caliper bar. No organic solutions are allowed.
- (3) Check to see if all the buttons, and LCD display respond well.

2. Basic measuring methods;


- (1) Loosen the locking screw.
- (2) Switch the unit on with a press on "ON" button. Then select the unit system needed by pressing Inch/Metric button. (Each time the button is pressed, inch and metric digits will be displayed alternatively).
- (3) Apply normal measuring pressure on slider to close the external measuring jaws. Then press "zero" button to reset the display to zero.

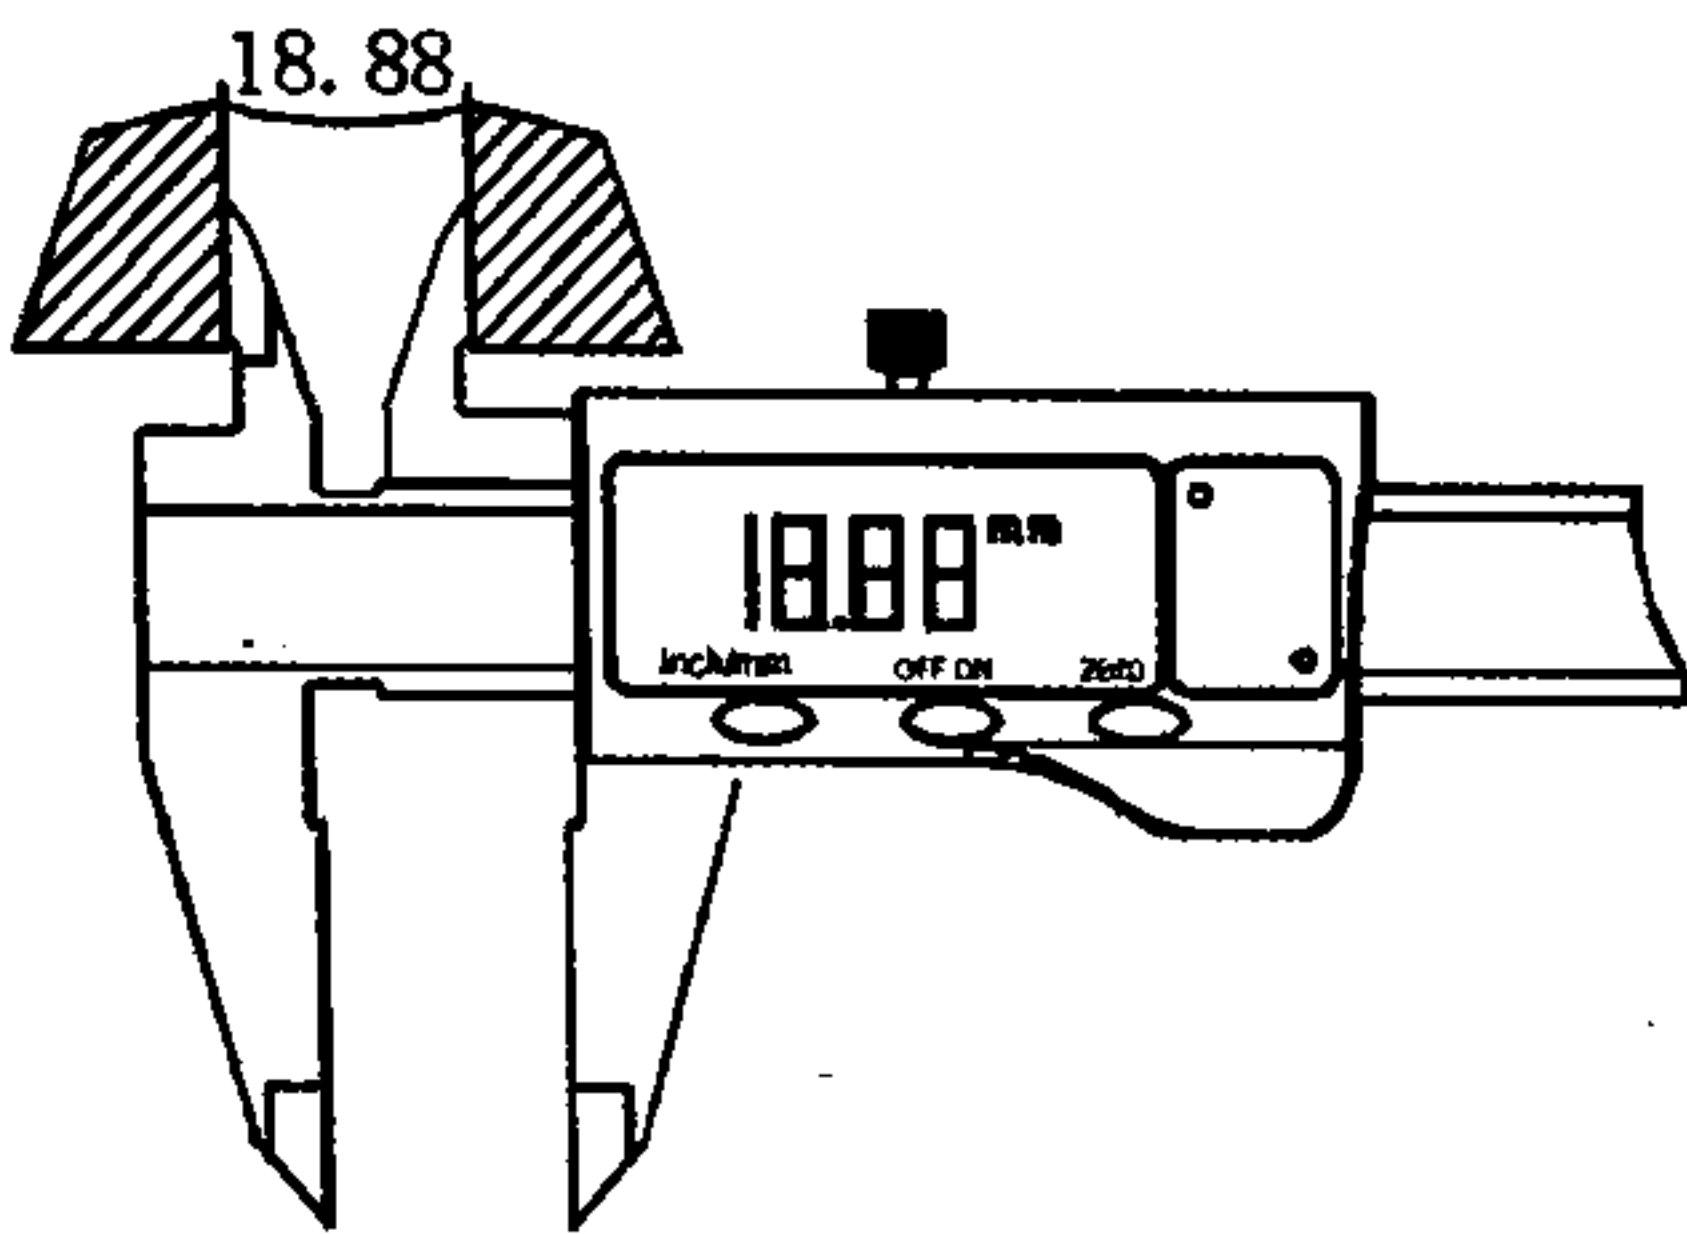


A. Measurements of internal dimensions

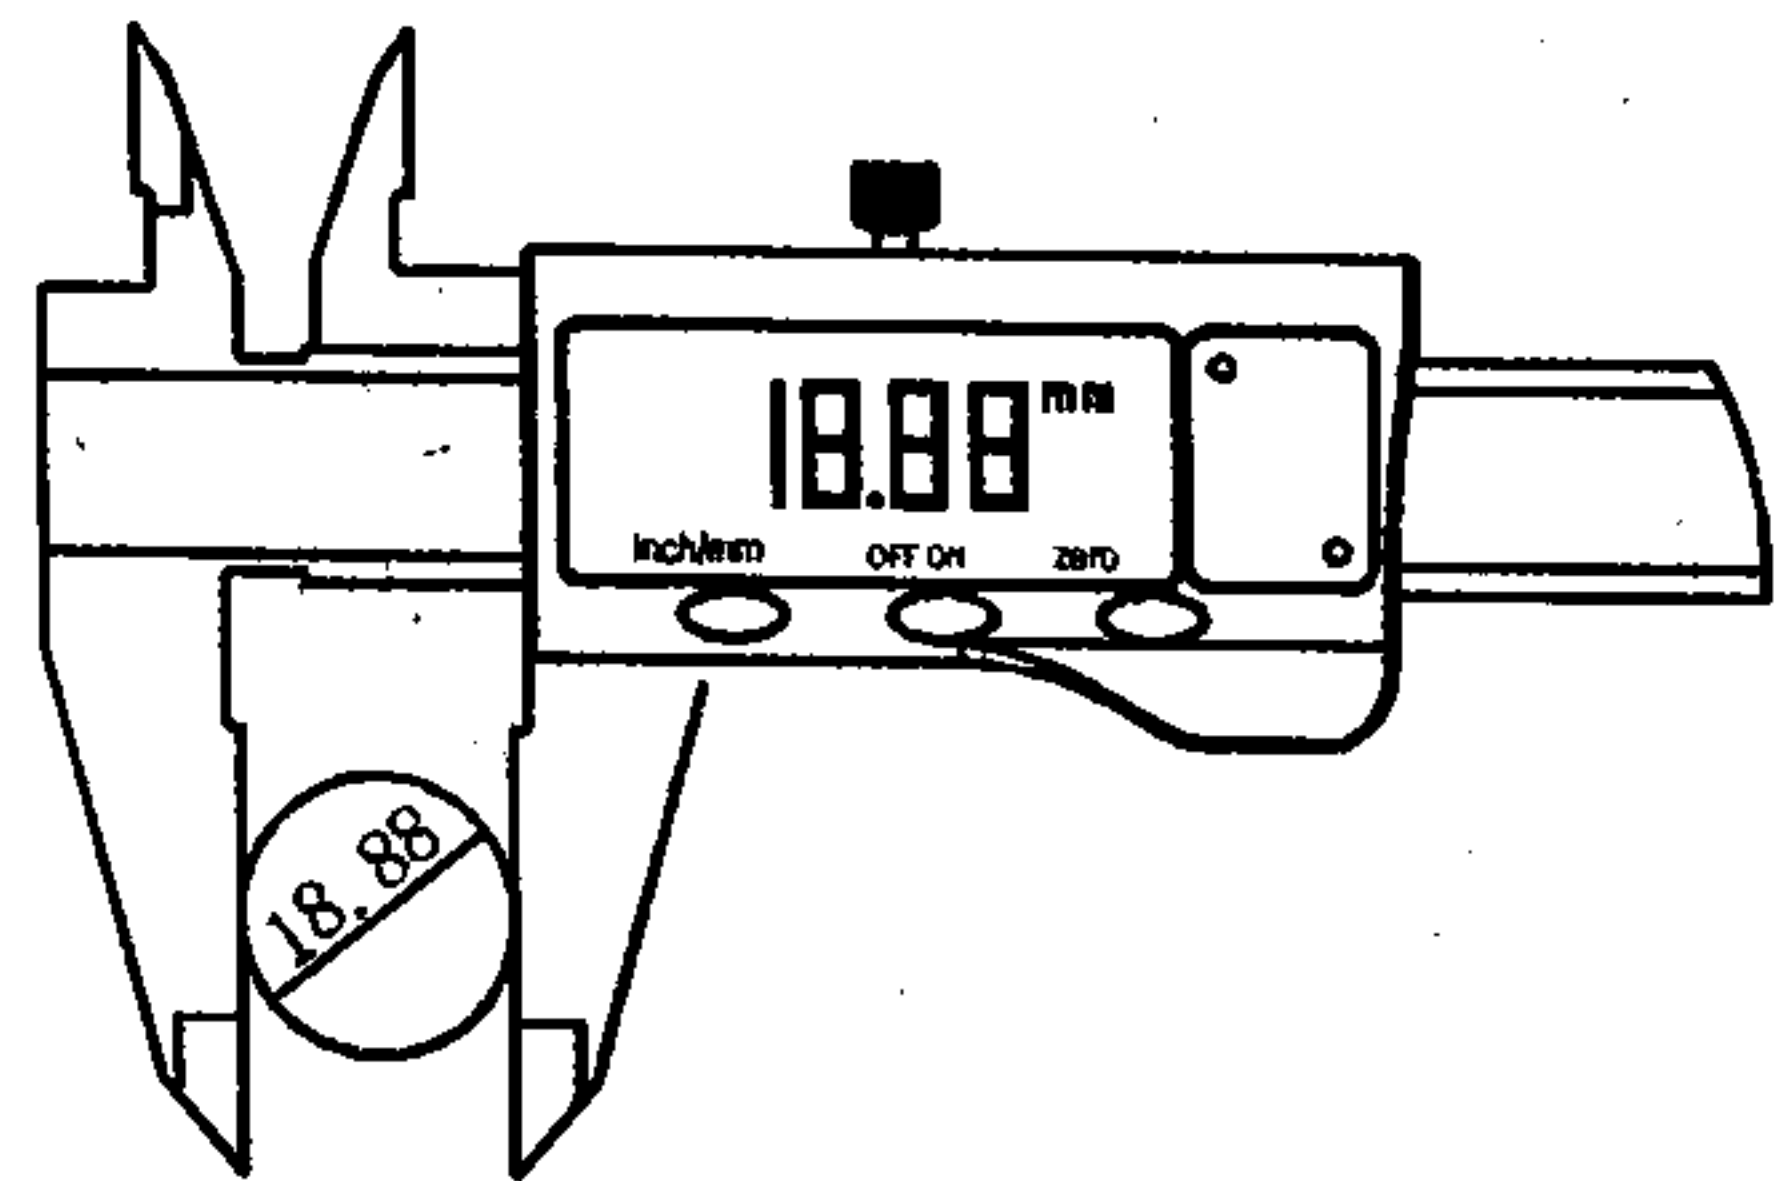

B. Measurements of external dimensions

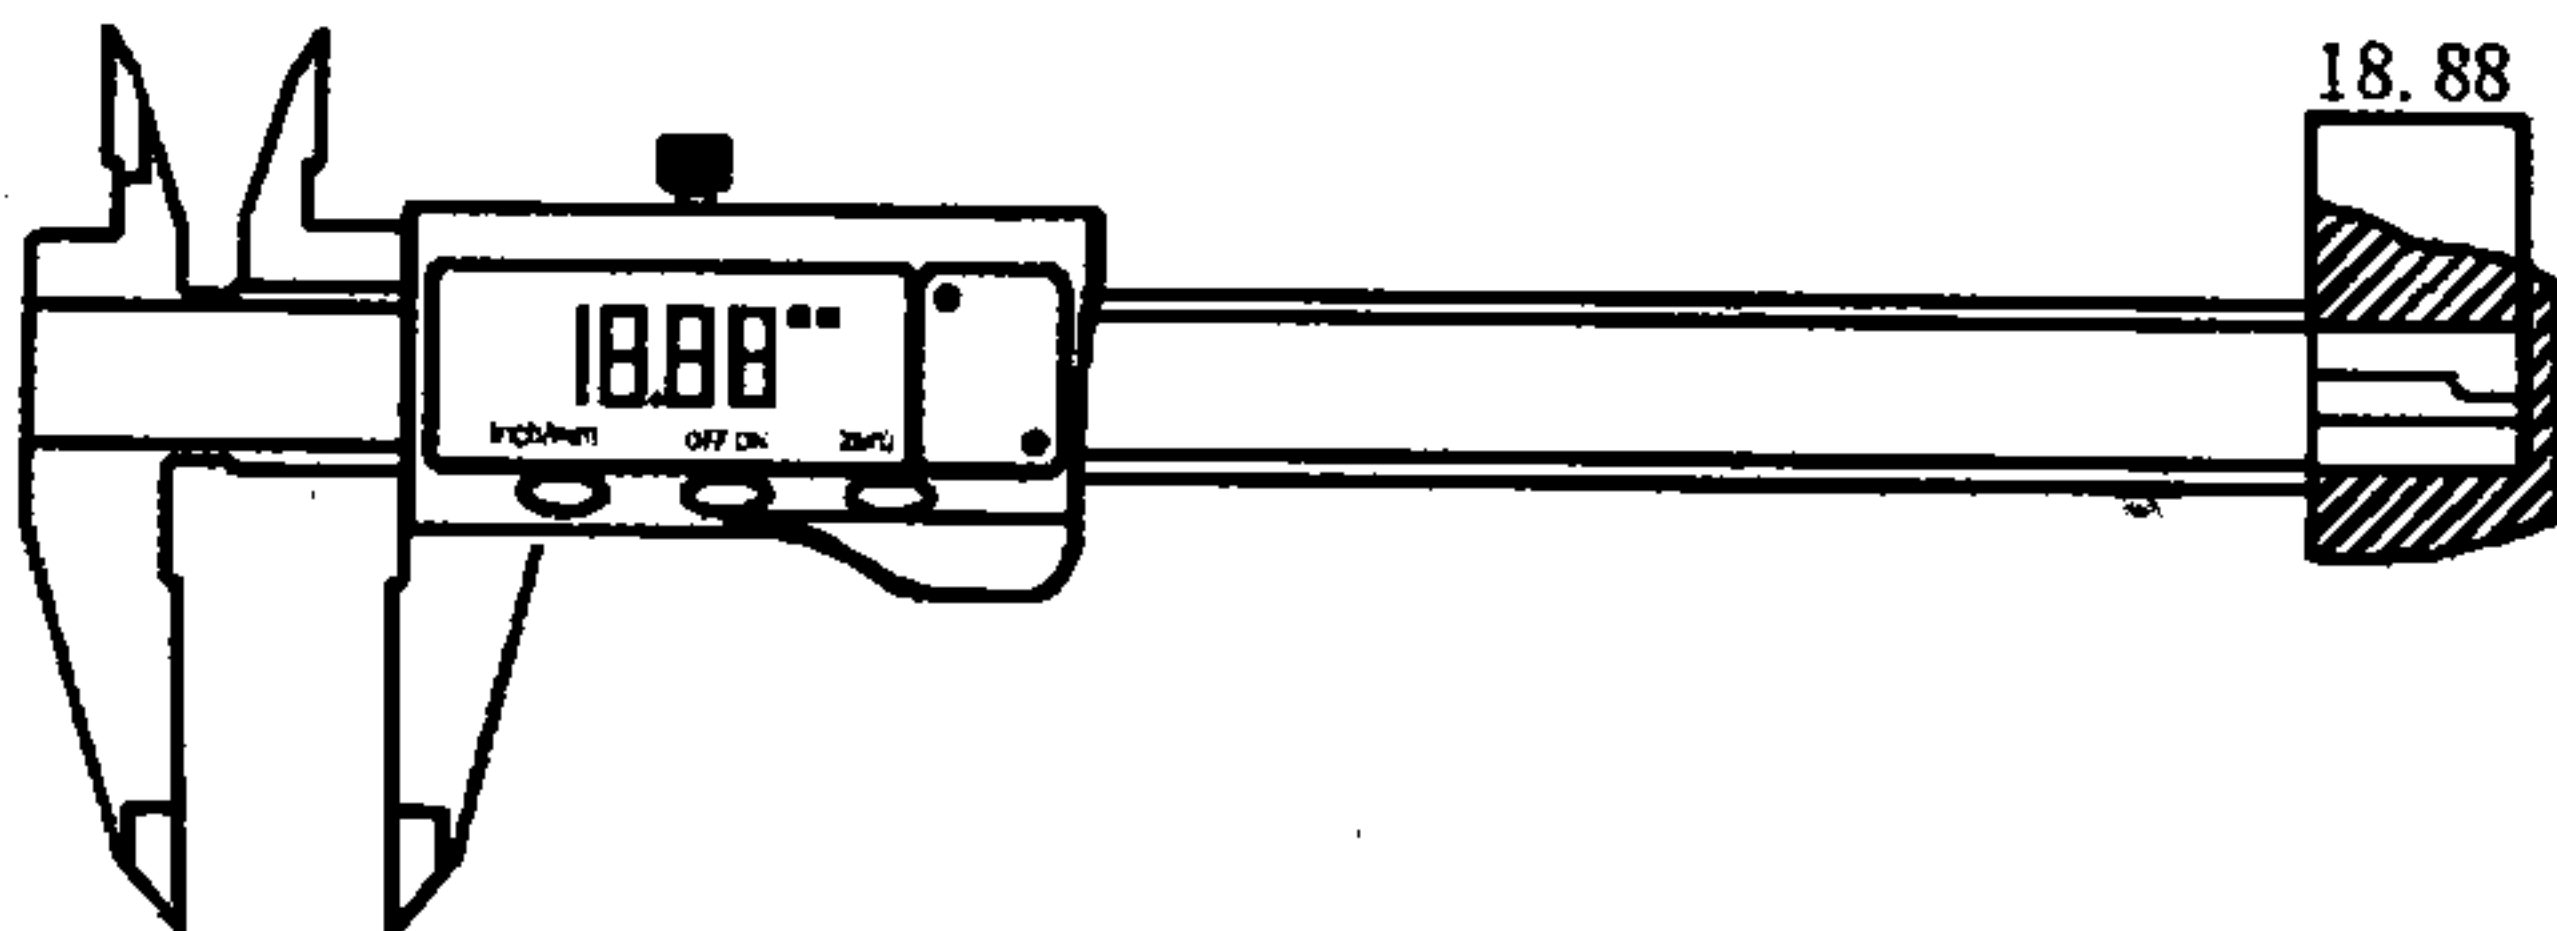


C. Measurements of depth

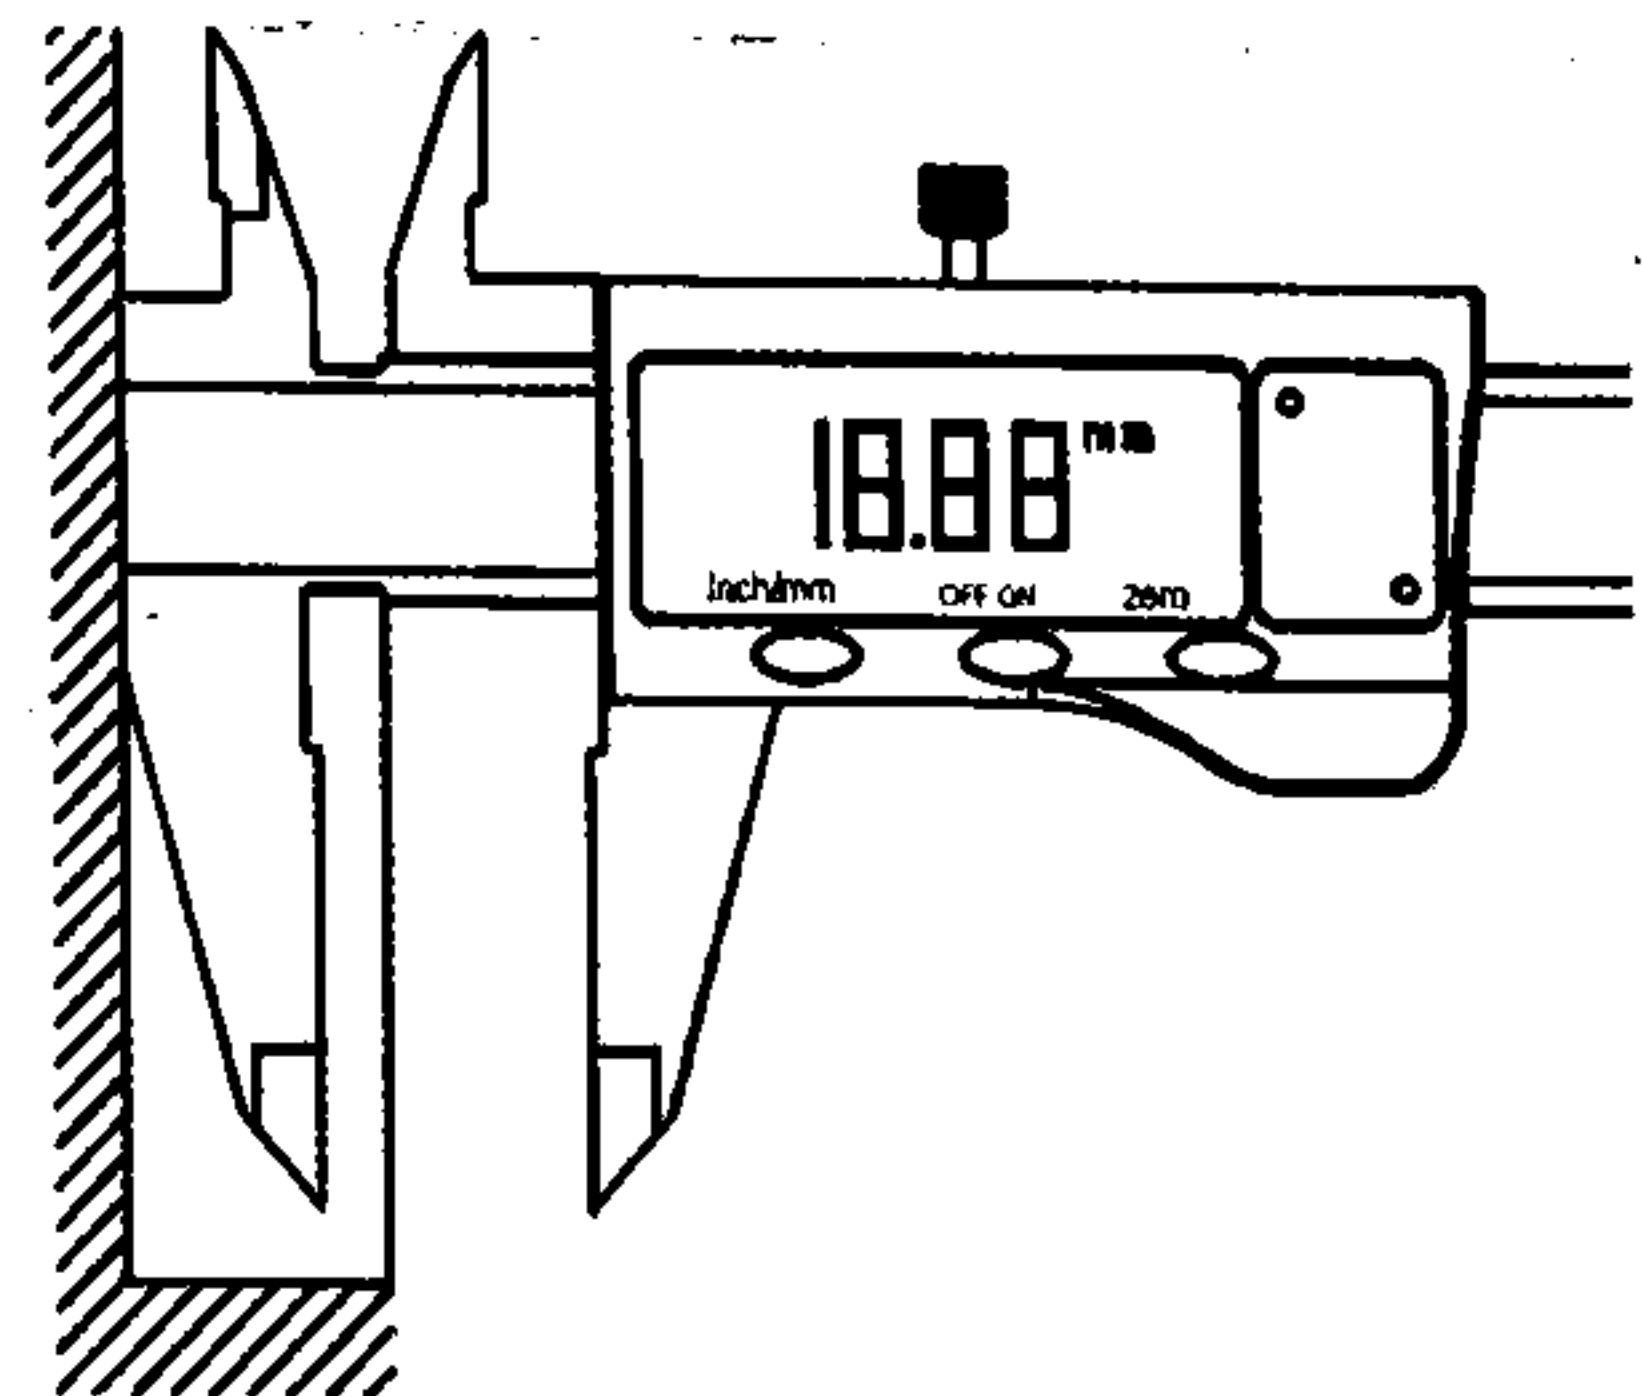


D. Measurements of steps

**E. Differential method of measurement
(Application of zero setting)**

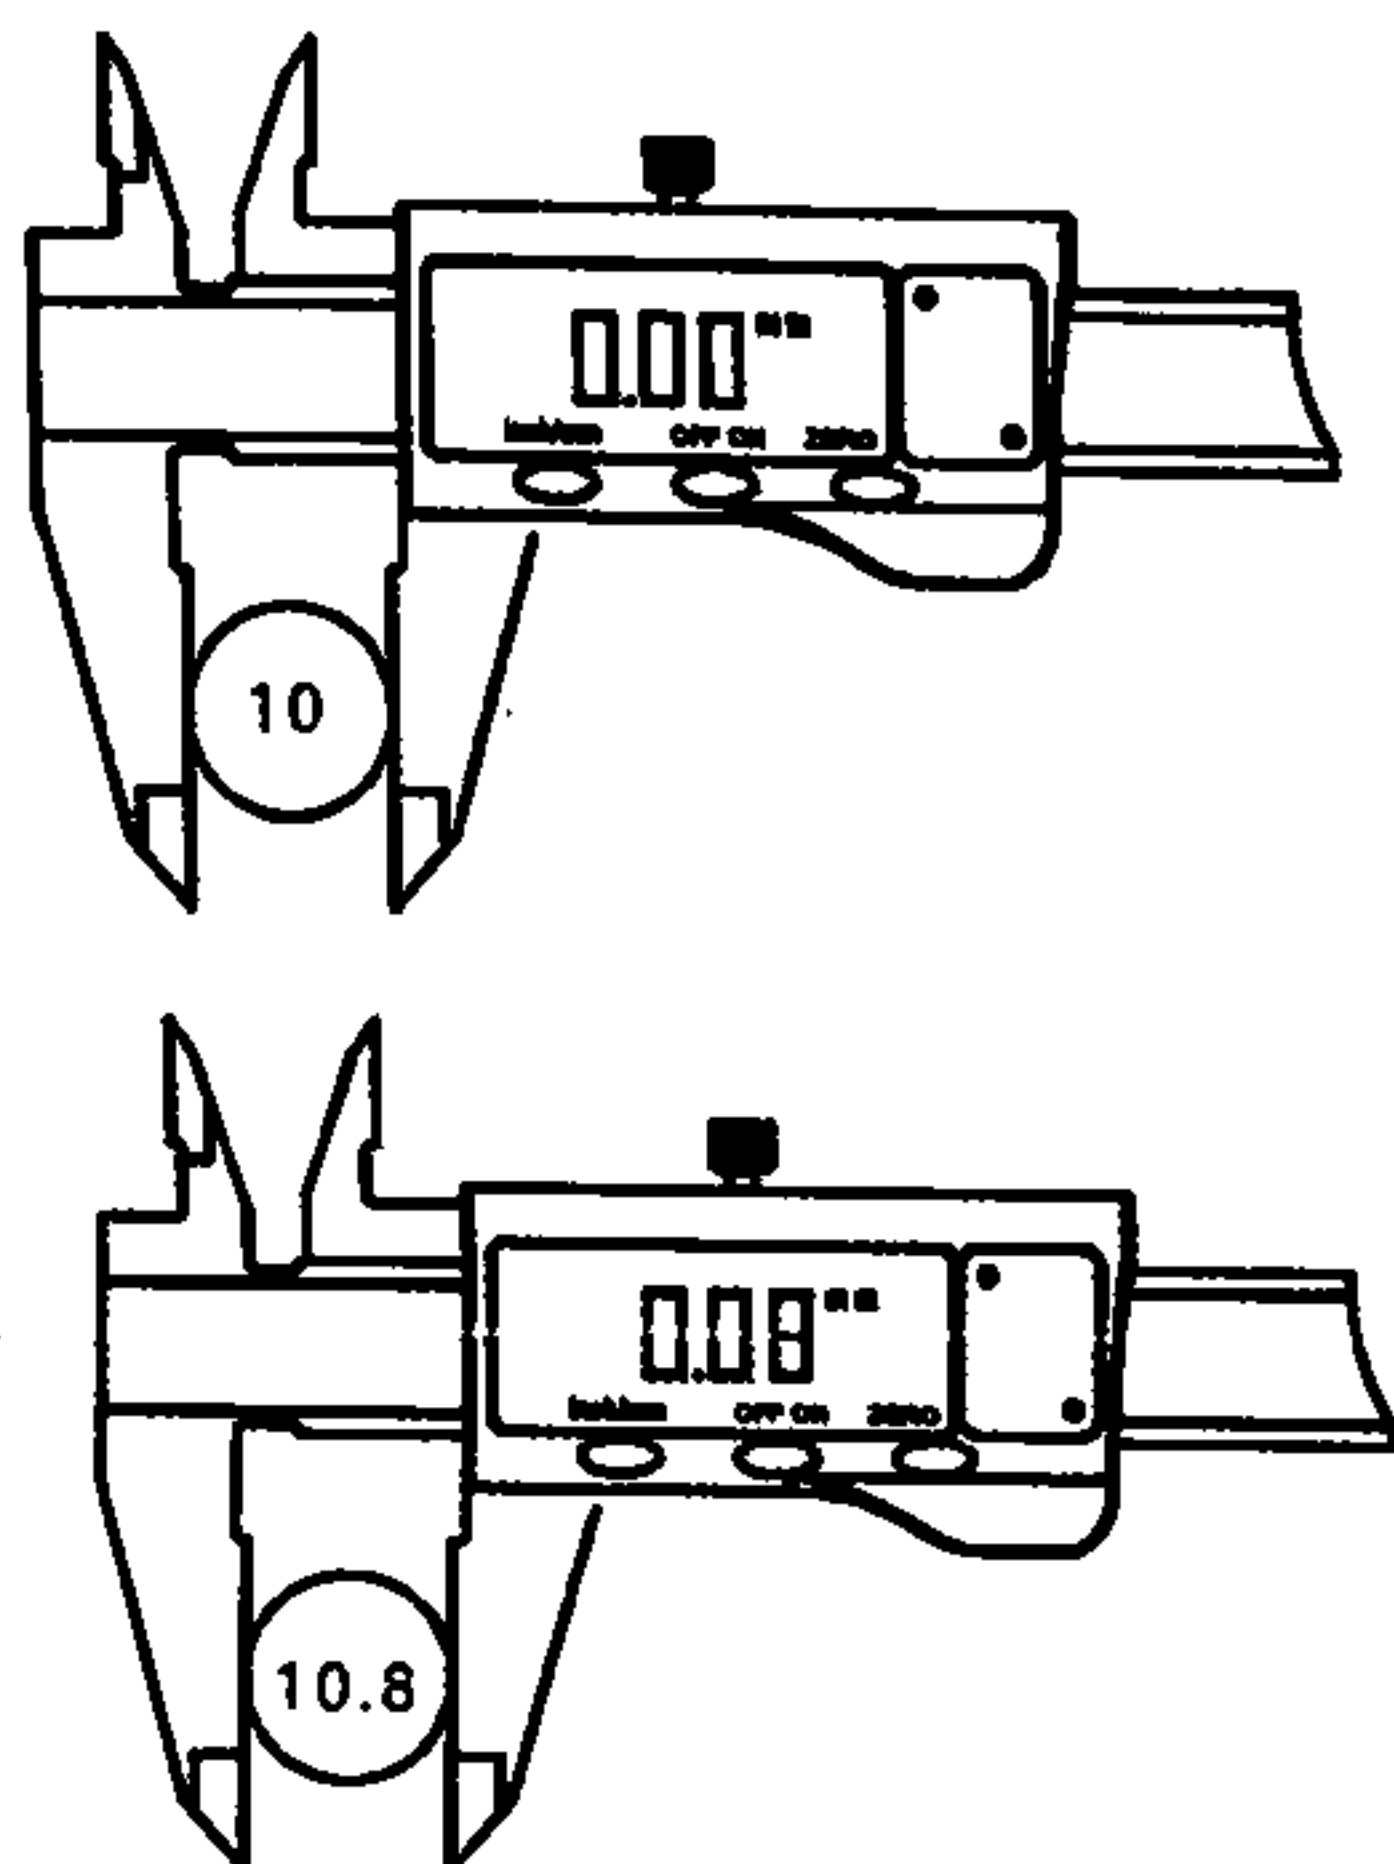

●NOMENCLATURE

- 1.Internal measuring jaws
- 2.METRIC/INCH/FAC change over
- 3.Locking screw
- 4.LCD display
- 5.External measuring jaws
- 6.Power on/off button
- 7.Zero setting
- 8.Battery cover
- 9.Depth measuring blade
- 10.Step-measuring faces

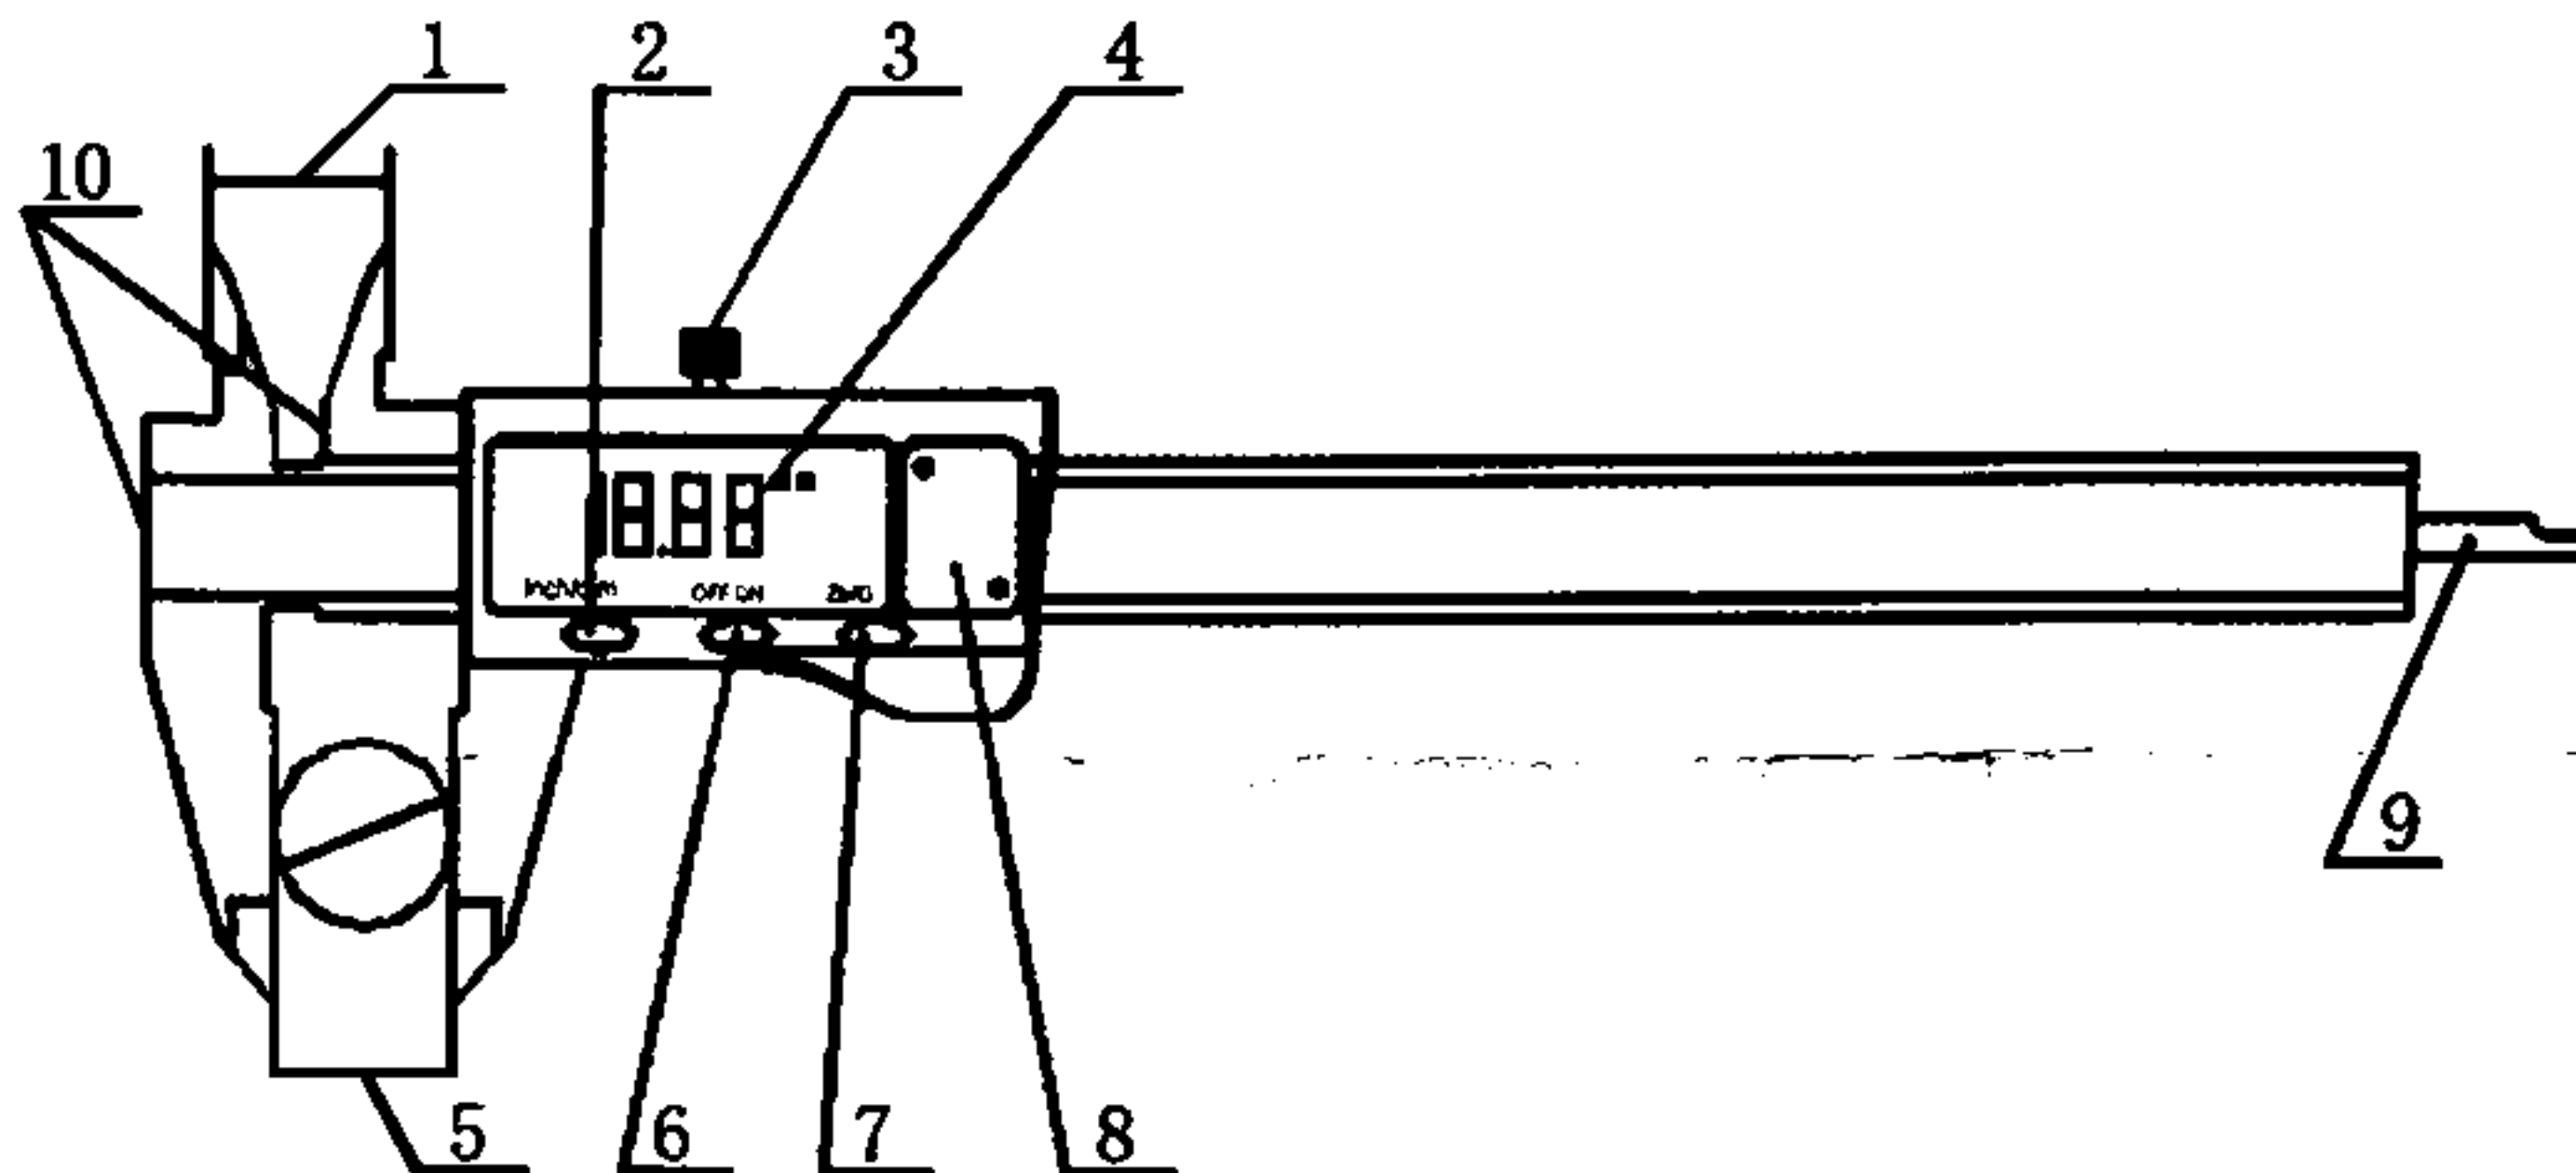

●TROUBLE SHOOTING

Failure	Cause	Measure
Display doesn't change when the slider is moved	Accidental trouble in circuit	Take out battery and reset it after 30 secretary
Less accurate than specified but within $\pm 0.1\text{mm}$	Dirt in the Sensor.	Remove slider cover and its assembly, clean face of sensor with clean compressed air ($5\text{kg}/\text{cm}^2$).
No display on LCD or less accurate than specified and more than $\pm 0.1\text{mm}$ or the numbers on the screen jump randomly	1. Battety in poor contact. 2. Battery voltage under 1.4V	1. Remove battery cover and adjust the battery seat, keep good connection. 2. Replace battery.

●MAINTENANCE INSTRUCTIONS

1. Clean caliper bar with dry cotton fabrics before using in order to avoid mad display of caliper caused by humidity.
2. Keep the caliper clean and dry (Liquid can damage the slider).
3. Faces should be cleaned gently with cotton fabrics, Never use petrol, acetone and other organic solutions.
4. In order to save power, turn off the unit when caliper is going to stay idle for some time.
5. Never apply any electric pressure on any part of the caliper and never use an electric pen for the fear of damaging its chip.
6. For other notes please refer to the conventional calipers.
7. Accidental wrong display may happen while replacing the battery. Just take out the battery and then put it in again after more than 30 seconds until the display returns to normal.

●WARNING:

"Immediately dispose of used batteries and keep away from children. Do NOT dispose of batteries in household trash."
 "Even used batteries may cause severe injury or death."
 "Call a local poison control center for treatment information."

●BATTERY REPLACEMENT

Flashing of digits shows a flat battery. Take off the battery cover in the direction shown by the arrow and replace the battery (positive side facing out).

